HANDMOTION.

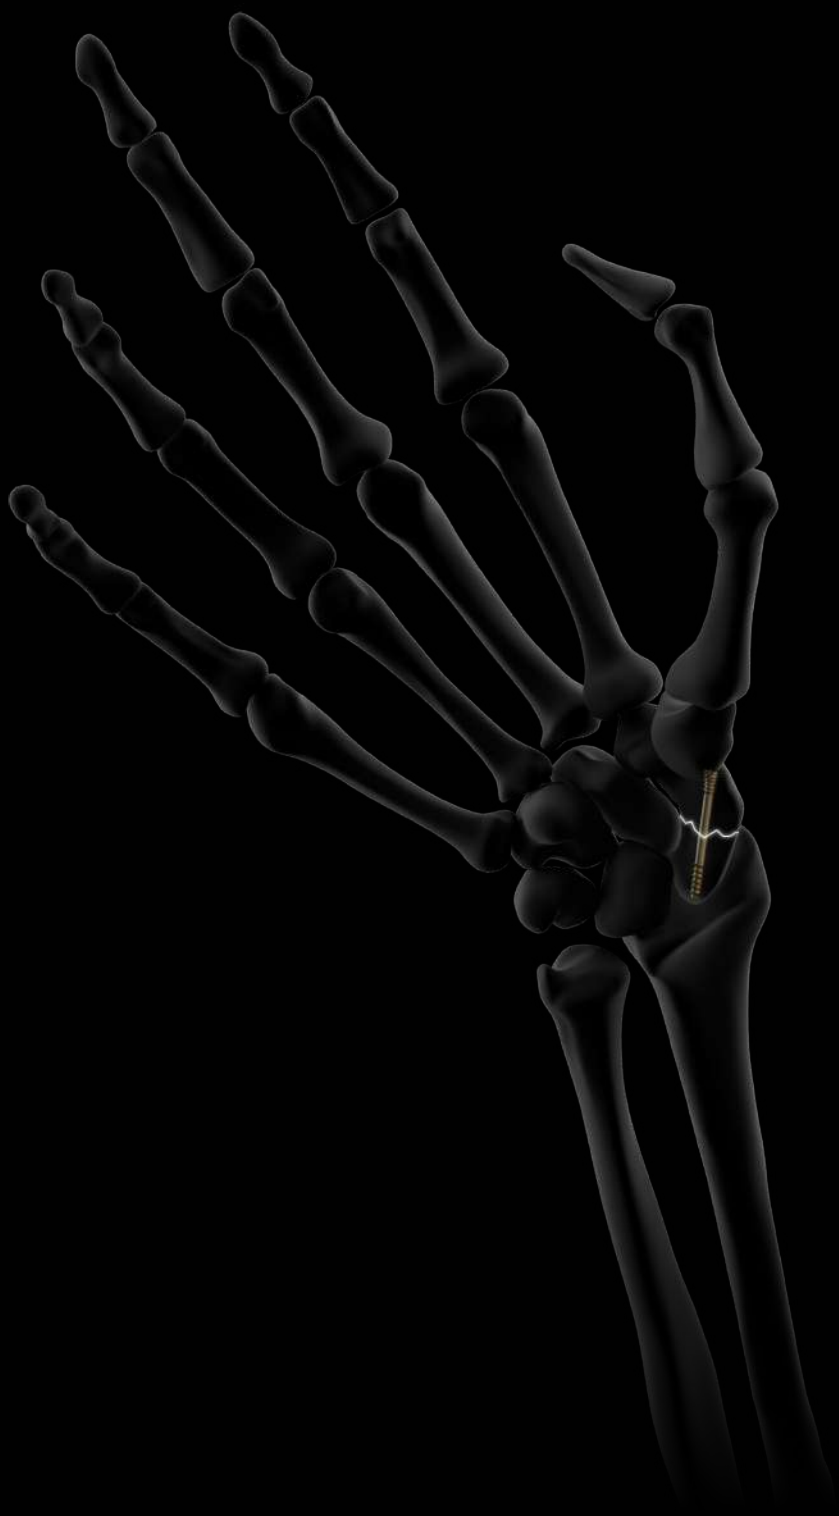

STAND-ALONE
SCREWS

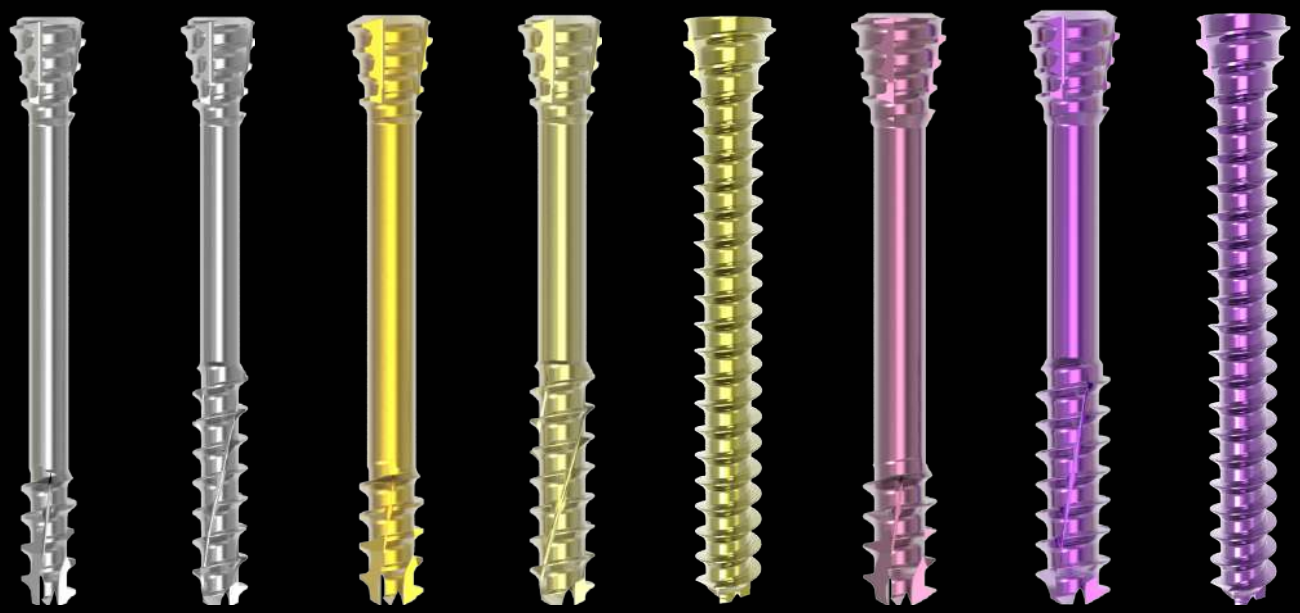

Handmotion.

STAND-ALONE SCREWS

Intended purpose:
Implants of the Stand-Alone Screws range are intended for fractures fixation, osteotomies and arthrodeses of bones in adults, appropriate for the size of the device.

Contraindications:
- Pregnancy.
- Acute or chronic local or systemic infections.
- Allergy to one of the materials used or sensitivity to foreign bodies.

Technical features.

- Available in sterile and non-sterile version
- Material: TA6V

Cannulated screws

Cylindro-conical profile of the head

Self-drilling
& self-tapping

3 TYPES OF THREADS

SHORT THREADED SCREW

FULLY THREADED SCREW

LONG THREADED SCREW

3 DIAMETERS

Ø2.25MM

Ø2.6MM

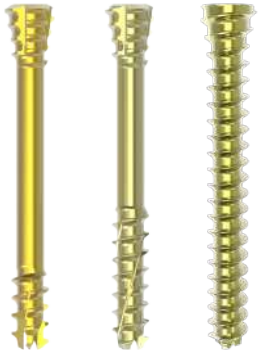

Ø3.0MM

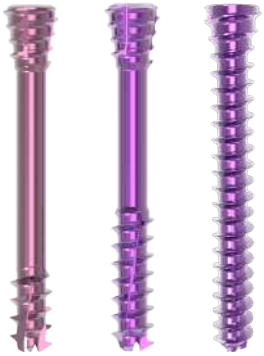

Implant references.

Please note that all implants are also available in sterile packaging. An "-ST" code is added at the end of the reference.
Ex : «H1.1IFT2.6L14-ST»

Ø2.25 mm Canulated screws*

Ref.	Description
H0.9IFT2.25Lxx	Ø2.25 mm self-compressive screw - cannula Ø0.9 - short thread L14 to L34 mm (2 mm increments)
H0.9HFT2.25Lxx	Ø2.25 mm self-compressive screw - cannula Ø0.9 - long thread L12 to L34 mm (2 mm increments)

*Non anodized

Ø2.6 mm Cannulated screws

Ref.	Description
H1.1IFT2.6Lxx *	Ø2.6 mm self-compressive screw - cannula Ø1.1 - short thread L14 to L34 mm (2 mm increments)
H1.1HFT2.6Lxx **	Ø2.6 mm self-compressive screw - cannula Ø1.1 - long thread L10 to L34 mm (2 mm increments)

*Gold anodized
**Yellow anodized

Ø3.0 mm Cannulated screws

Ref.	Description
H1.1IFT3.0Lxx *	Ø3.0 self-compressive screw - cannula Ø1.1 - short thread L14 to L34 mm (2 mm increments)
H1.1HFT3.0Lxx **	Ø3.0 self-compressive screw - cannula Ø1.1 - long thread L10 to L40 mm (2 mm increments)

*Pink anodized
**Fuschia anodized

Ø2.6 mm Cannulated screws*

Ref.	Description
H1.1GFT2.6Lxx	Ø2.6 mm neutralization screw - cannula Ø1.1 - full thread L10 to L34 mm (2 mm increments)

*Yellow anodized

Ø3.0 mm Cannulated screws*

Ref.	Description
H1.1GFT3.0Lxx	Ø3.0 mm neutralization screw - cannula Ø1.1 - full thread L10 to L40 mm (2 mm increments)

*Fuschia anodized



Instrument references.

Instruments

Ref.	Screw	Description
ANC104	●	1.5 mm quick coupling hexagonal prehensor screwdriver - cannula Ø0.9 mm
ANC105	●	Ø0.8 mm Pin guide
ANC106	●	Ø1.7 mm quick coupling drill bit - cannula Ø0.9 mm
ANC108	● ●	Length gauge for pin Ø1.0 mm - L150 mm
ANC125	●	Ø1.0 mm pin guide
ANC135	●	Ø2.0 mm quick coupling drill bit - cannulated Ø1.1 mm
ANC137	●	Ø2.2 mm quick coupling drill bit - cannulated Ø1.1 mm
ANC139	●	2.0 mm quick coupling hexagonal prehensor screwdriver - cannula Ø1.1 mm
ANC140	●	Ø1.7 mm countersink - cannula Ø0.9 mm
ANC141	●	Ø2.0 mm countersink - cannula Ø1.1 mm
ANC142	●	Ø2.2 mm countersink - cannula Ø1.1 mm
ANC144		16cm forceps
ANC148	●	1.8 mm quick coupling hexagonal prehensor screwdriver - cannula Ø1.1 mm
ANC165		Prehensive plier for screws
ANC166	●	Pins support for Ø0.8 mm pin
ANC166L	● ●	Pins support for Ø0.8 mm pin - Long
ANC167	● ●	Pins support for Ø1.0 mm pin
ANC167L	●	Pins support for Ø1.0 mm pin - Long
ANC224		Length gauge Hand/Footv
ANC699	●	3-in-1 instrument for Ø2.25 mm screws
ANC700	●	3-in-1 instrument for Ø2.6 mm screws
ANC701	●	3-in-1 instrument for Ø3.0 mm screws
ANC350	● ●	Ø4.5 mm AO quick coupling handle - Size 1
33.0208.150		Pin Ø0.8 - L150 mm
33.0210.150		Pin Ø1.0 - L150 mm

Extremity metacarpal screws fixation options *

Ref.	Description	Compatible with screws
ANC1352	2-in-1 instrument for Ø2.6 mm screws	H1.1GFT2.6Lxx - L10 to L34 mm (2mm increments)
ANC1353	2-in-1 instrument for Ø3.0 mm screws	H1.1GFT3.0Lxx - L10 to L40 mm (2mm increments)

* Available on demand only

Container references.

Containers

Ref.	Description
ANC154	Footmotion / Handmotion instrumentation set
ANC155/CB	Footmotion / Handmotion set – Cambered lid
ANC155	Footmotion / Handmotion implants set
ANC155/C	Footmotion / Handmotion set - Lid
ANC539/R	Handmotion instrumentation set - Screw rack
ANC208/R	Footmotion instrumentation set - Screw rack

This information is intended to demonstrate the Newclip Technics portfolio of medical devices. Always refer to the package insert, product label and/or user instructions including cleaning and sterilization before using any Newclip Technics product.These products must be handled and/or implanted by trained and qualified staff who have read the instructions before use. A surgeon must always rely on her or his own professional clinical judgement when deciding whether to use a particular product when treating a particular patient. Product availability is subject to the regulatory or medical practices that govern individual markets. Please contact your Newclip Technics representative if you have questions about the availability of Newclip Technics products in your area.

Manufacturer : Newclip Technics – Brochure EN – HANDMOTION – ED8 – 09/2026 - Medical device EC: class IIb – CE1639 SGS BE
Read labelling and instructions before the use of Newclip Technics medical devices. These products must be handled and/or implanted by trained and qualified staff who have read the instructions before use.
Non-contractual pictures.
Newclip Technics - 45 rue des Garottières - 44115 Haute Goulaine, France. Our subsidiaries: Newclip USA - Newclip Australia - Newclip Germany - Newclip Japan - Newclip Iberia - Newclip Belgium - Newclip Italia.

newcliptechnics.com